


SAMPLE INFORMATION

Sample Name:	SA002/APB/A03/35	Acquired By:	Manikanta.B
Sample Type:	Unknown	Sample Set Name:	07012026 HPLC 04 APB S001
Vial:	1:F,1	Acq. Method Set:	APB A02 A03 RS MTH
Injection #:	1	Processing Method:	08012026_HPLC_04_APB_P008
Injection Volume:	10.00 ul	Channel Name:	2998 Ch1 308nm@4.8nm
Run Time:	30.0 Minutes	Proc. Chnl. Descr.:	2998 Ch1 308nm@4.8nm
Date Acquired:	07-01-2026 23:23:34 IST	Column_ID:	NAL-ARD-LC-2025-017
Date Processed:	08-01-2026 09:24:39 IST	AR.Number	COA/2601/003
Batch Number:	SA002/APB/A03/35	Instrument ID:	NAL_ARD_HPLC_04_PDA

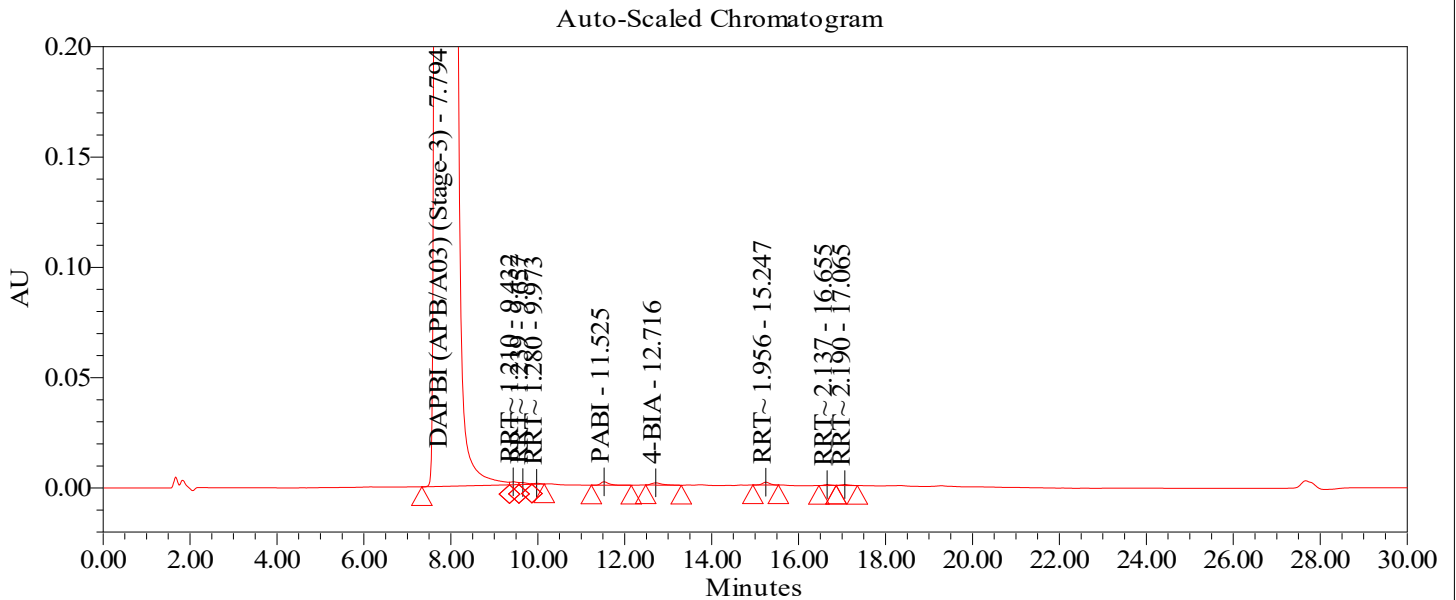

AR_Number COA/2601/003; Batch_Number SA002/APB/A03/35; Processed Channel Descr. 2998 Ch1 308nm@4.8nm; Processed By Raju/Analyst; Result # 1; Result Id 2562

Peak Results

	Name	RT	Height (μV)	Area	% Area	RT Ratio
1	DAPBI (APB/A03) (Stage-3)	7.794	3164666	71394752	99.87	1.00
2	RRT~ 1.210	9.432	1311	15542	0.02	1.21
3	RRT~ 1.239	9.657	886	11575	0.02	1.24
4	RRT~ 1.280	9.973	426	4593	0.01	1.28
5	PABI	11.525	1577	20118	0.03	1.48
6	4-BIA	12.716	1014	17183	0.02	1.63
7	RRT~ 1.956	15.247	1292	15254	0.02	1.96

Peak Results

	Name	RT	Height (μ V)	Area	% Area	RT Ratio
8	RRT~ 2.137	16.655	389	4266	0.01	2.14
9	RRT~ 2.190	17.065	401	5166	0.01	2.19

Result Sign Off

	SampleName	Result Id	Sign Off Full Name	Sign Off Date
1	SA002/APB/A03/35	2562	Raju.A (RAJU)	08-01-2026 10:15:37 IST
2	SA002/APB/A03/35	2562	Jayendra kiran K. (jkiran)	08-01-2026 10:35:27 IST

Result Sign Off

	Sign Off Reason
1	Sign Off Level 1, Reason: Data Submitted for review
2	Sign Off Level 2, Reason: Review

System Name NAL_ARD_HPLC_04_PDA