


SAMPLE INFORMATION

Sample Name:	DA003-PPA/A03/024 wet solid	Acquired By:	Raja
Sample Type:	Unknown	Sample Set Name:	30102025_HPLC_03_S001
Vial:	1:E,3	Acq. Method Set:	30102025_HPLC_03_M002_MTH
Injection #:	1	Processing Method:	30102025_HPLC_03_P011
Injection Volume:	10.00 ul	Channel Name:	W2489 ChA
Run Time:	41.0 Minutes	Proc. Chnl. Descr.:	W2489 ChA 213nm
Date Acquired:	30-10-2025 22:14:32 IST	Column_ID:	NAL-ARD-LC-2024-001
Date Processed:	31-10-2025 06:22:10 IST	AR.Number	ARD/HPLC/2510/1210
Batch Number:	DA003-PPA/A03/024	Instrument ID:	NAL_ARD_HPLC_03

METHOD INFORMATION:

Column name: XBridge C18(4.6x150mm) 3.5µm
 Mobile phase A: 10mm Ammonium Bicarbonate Ph-8.7
 Mobile phase B: MeOH;ACN(1;1) V/V
 Gradient (%B) :0/15,3/15,25/80,35/80,36/15,41/15.
 Column Temp :40°C
 Sample Temp :25°C
 Wavelength :213nm
 Run time :41 min

Auto-Scaled Chromatogram

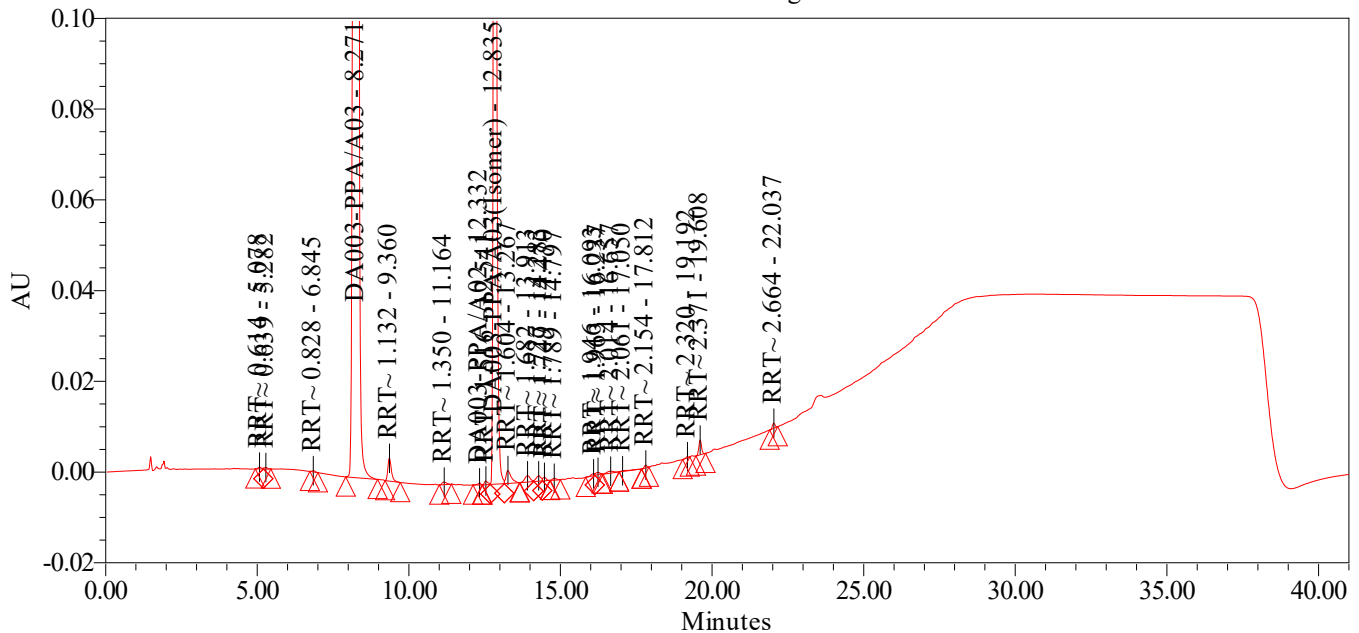

Peak Results

	Name	RT	Height (µV)	Area	% Area	RT Ratio
1	RRT~ 0.614	5.078	392	3081	0.03	0.614
2	RRT~ 0.639	5.282	347	2654	0.03	0.639

Reported by User: Satyanarayana Menti (Satya)

Report Method: General Report_01_PPA__3

Report Method ID: 5785

Page: 1 of 2

Project Name: 2025\October\NAL_ARD_HPLC_03

Date Printed:

31-10-2025

09:02:47 Asia/Kolkata

Peak Results

	Name	RT	Height (μ V)	Area	% Area	RT Ratio
3	RRT~ 0.828	6.845	266	2054	0.02	0.828
4	DA003-PPA/A03	8.271	982187	8075175	79.59	1.000
5	RRT~ 1.132	9.360	5063	41139	0.41	1.132
6	RRT~ 1.350	11.164	579	6101	0.06	1.350
7	DA003-PPA/A02	12.332	460	3027	0.03	1.491
8	RRT~ 1.516	12.541	828	6672	0.07	1.516
9	DA003-PPA/A03(Isomer)	12.835	282948	1881254	18.54	1.552
10	RRT~ 1.604	13.267	2843	34259	0.34	1.604
11	RRT~ 1.682	13.913	1383	17969	0.18	1.682
12	RRT~ 1.727	14.283	1218	13216	0.13	1.727
13	RRT~ 1.749	14.470	778	6041	0.06	1.749
14	RRT~ 1.789	14.797	410	3505	0.03	1.789
15	RRT~ 1.946	16.093	379	3278	0.03	1.946
16	RRT~ 1.963	16.237	491	4670	0.05	1.963
17	RRT~ 2.014	16.657	430	6942	0.07	2.014
18	RRT~ 2.061	17.050	174	3604	0.04	2.061
19	RRT~ 2.154	17.812	640	3712	0.04	2.154
20	RRT~ 2.320	19.192	223	1194	0.01	2.320
21	RRT~ 2.371	19.608	3289	20277	0.20	2.371
22	RRT~ 2.664	22.037	1139	6769	0.07	2.664

Result Sign Off

	SampleName	Result Id	Sign Off Full Name
1	DA003-PPA/A03/024 w et solid	6335	Satyanarayana Menti (satya)
2	DA003-PPA/A03/024 w et solid	6335	Ramanjaneyulu Gadiparthi (ramanjaneyulu)

Result Sign Off

	Sign Off Date	Sign Off Reason
1	31-10-2025 06:23:56 IST	Sign Off Level 1, Reason: Data Submitted for review
2	31-10-2025 08:29:42 IST	Sign Off Level 2, Reason: Review

System Name NAL_ARD_HPLC_03

Reported by User: Satyanarayana Menti (Satya)

Report Method: General Report_01_PPA__3

Report Method ID: 5785

Page: 2 of 2

Project Name: 2025\October\NAL_ARD_HPLC_03

Date Printed:

31-10-2025

09:02:47 Asia/Kolkata