


SAMPLE INFORMATION

Sample Name:	SA-002/APB/A02/053	Acquired By:	Analyst
Sample Type:	Unknown	Sample Set Name:	06012026_HPLC_03_APB_S001
Vial:	1:F,8	Acq. Method Set:	APB_A02_A03_RS_MTH
Injection #:	1	Processing Method:	06012026_HPLC_03_APB_P021
Injection Volume:	10.00 ul	Channel Name:	W2489 ChA
Run Time:	30.0 Minutes	Proc. Chnl. Descr.:	W2489 ChA 308nm
Date Acquired:	06-01-2026 18:22:38 IST	Column_ID:	NAL-ARD-LC-2025-017
Date Processed:	06-01-2026 20:55:07 IST	AR.Number	NA
Batch Number:	SA-002/APB/A02/053	Instrument ID:	NAL_ARD_HPLC_03

METHOD INFORMATION:

Column name: X-Terra RP18(4.6x150mm) 5µm
 Mobile phase A:20mm Ammonium bi carbonate 1000ml H2O pH-8.0
 Mobile phase B:Methanol
 Gradient (%B) :0/15,2/15,20/90,25/90,25.1/15,30/15
 Column Temp :40°C
 Sample Temp :25°C
 Wavelength :308nm
 Run time : 30 min
 Flow rate :1.0mL/min

Auto-Scaled Chromatogram

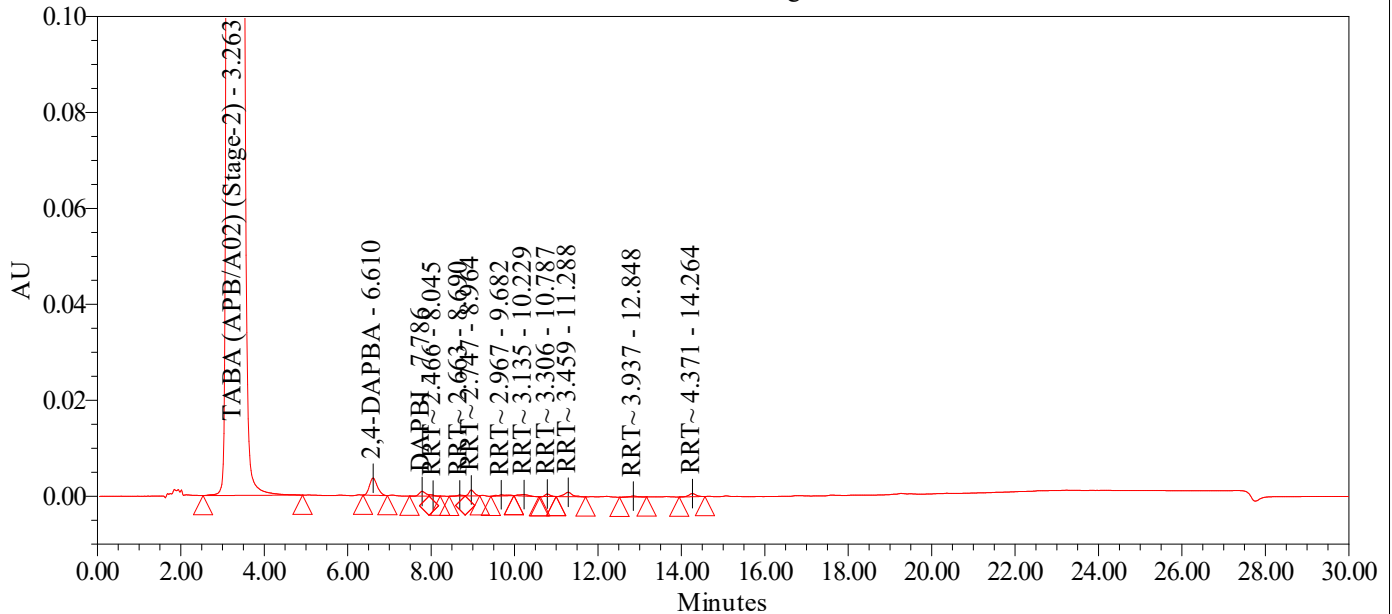

Peak Results

	Name	RT	Height (µV)	Area	% Area	RT Ratio
1	TABA (APB/A02) (Stage-2)	3.263	2151941	30894813	99.644	1.000
2	2,4-DAPBA	6.610	3589	46480	0.150	2.026

Peak Results

	Name	RT	Height (μ V)	Area	% Area	RT Ratio
3	DAPBI	7.786	1000	11133	0.036	2.386
4	RRT~ 2.466	8.045	224	2342	0.008	2.466
5	RRT~ 2.663	8.690	219	2131	0.007	2.663
6	RRT~ 2.747	8.964	1233	10968	0.035	2.747
7	RRT~ 2.967	9.682	245	4419	0.014	2.967
8	RRT~ 3.135	10.229	317	5132	0.017	3.135
9	RRT~ 3.306	10.787	551	4750	0.015	3.306
10	RRT~ 3.459	11.288	921	12575	0.041	3.459
11	RRT~ 3.937	12.848	211	2849	0.009	3.937
12	RRT~ 4.371	14.264	652	7591	0.024	4.371

Result Sign Off

	SampleName	Result Id	Sign Off Full Name
1	SA-002/APB/A02/053	1979	Manikanta.Bheemavarapu (manikanta.b)
2	SA-002/APB/A02/053	1979	Jayendra kiran K. (jkiran)

Result Sign Off

	Sign Off Date	Sign Off Reason
1	06-01-2026 20:55:31 IST	Sign Off Level 1, Reason: Data Submitted for review
2	07-01-2026 09:09:48 IST	Sign Off Level 2, Reason: Review

System Name NAL_ARD_HPLC_03