


SAMPLE INFORMATION

Sample Name:	DA004-DNT/A04/038 A/W O.L	Acquired By:	Raju
Sample Type:	Unknown	Sample Set Name:	04102025_HPLC_04_S001
Vial:	1:D,1	Acq. Method Set:	04102025_HPLC_04_M001_MTH
Injection #:	1	Processing Method:	04102025_HPLC_04_P013
Injection Volume:	10.00 ul	Channel Name:	2998 Ch1 225nm@4.8nm
Run Time:	35.0 Minutes	Proc. Chnl. Descr.:	2998 Ch1 225nm@4.8nm
Date Acquired:	04-10-2025 14:53:02 IST	Column_ID:	NAL-ARD-LC-2025-011
Date Processed:	04-10-2025 16:09:26 IST	AR.Number	HPLC/2510/081
Batch Number:	DA004-DNT/A04/038 A/	Instrument ID:	NAL_ARD_HPLC_04_PDA

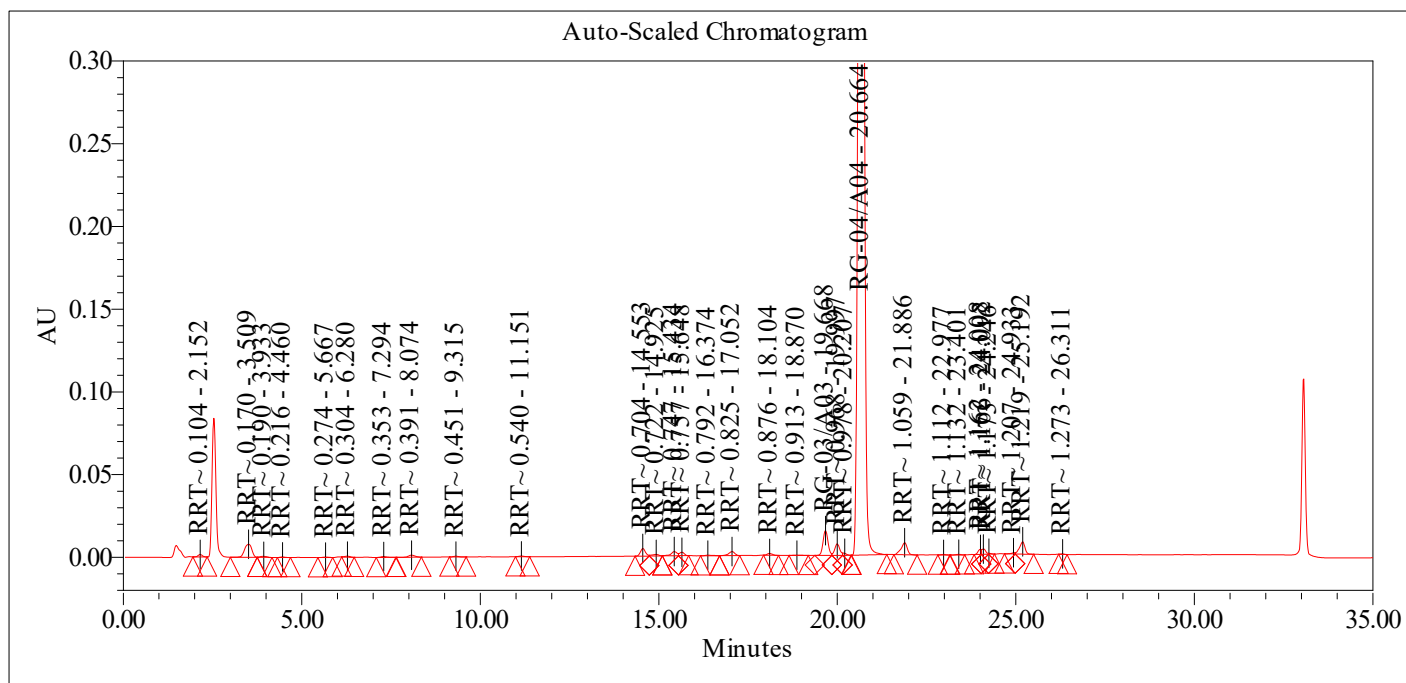

Peak Results

	Name	RT	Height (µV)	Area	% Area	RT Ratio
1	RRT~ 0.104	2.152	1498	12593	0.12	0.104
2	RRT~ 0.170	3.509	7871	111614	1.07	0.170
3	RRT~ 0.190	3.933	562	7293	0.07	0.190
4	RRT~ 0.216	4.460	354	2852	0.03	0.216
5	RRT~ 0.274	5.667	284	3441	0.03	0.274
6	RRT~ 0.304	6.280	605	5991	0.06	0.304
7	RRT~ 0.353	7.294	523	6015	0.06	0.353
8	RRT~ 0.391	8.074	1247	15728	0.15	0.391
9	RRT~ 0.451	9.315	489	4653	0.04	0.451

Reported by User: Manikanta.Bheemavarapu (Manikanta.B)

Report Method: General Report_DNT

Report Method ID: 1358

Page: 1 of 2

Project Name: 2025\October\NAL_ARD_HPLC_04

Date Printed:

04-10-2025

16:37:46 Asia/Kolkata

Peak Results

	Name	RT	Height (μ V)	Area	% Area	RT Ratio
10	RRT~ 0.540	11.151	401	3864	0.04	0.540
11	RRT~ 0.704	14.553	4625	44777	0.43	0.704
12	RRT~ 0.722	14.925	935	12053	0.12	0.722
13	RRT~ 0.747	15.434	2470	28669	0.27	0.747
14	RRT~ 0.757	15.648	2071	18934	0.18	0.757
15	RRT~ 0.792	16.374	411	5274	0.05	0.792
16	RRT~ 0.825	17.052	2433	28956	0.28	0.825
17	RRT~ 0.876	18.104	1076	10392	0.10	0.876
18	RRT~ 0.913	18.870	164	2869	0.03	0.913
19	RG-03/A03	19.668	15015	144931	1.39	0.952
20	RRT~ 0.968	19.997	6929	67859	0.65	0.968
21	RRT~ 0.978	20.207	1193	8854	0.08	0.978
22	RG-04/A04	20.664	1036632	9684695	92.59	1.000
23	RRT~ 1.059	21.886	7238	88022	0.84	1.059
24	RRT~ 1.112	22.977	307	2874	0.03	1.112
25	RRT~ 1.132	23.401	367	3545	0.03	1.132
26	RRT~ 1.162	24.008	2986	18335	0.18	1.162
27	RRT~ 1.166	24.092	3243	25381	0.24	1.166
28	RRT~ 1.173	24.246	487	2487	0.02	1.173
29	RRT~ 1.207	24.933	723	5506	0.05	1.207
30	RRT~ 1.219	25.192	7496	79371	0.76	1.219
31	RRT~ 1.273	26.311	306	1915	0.02	1.273

Result Sign Off

	SampleName	Result Id	Sign Off Full Name
1	DA004-DNT/A04/038 A/W O.L	2004	Manikanta.Bheemavarapu (manikanta.b)
2	DA004-DNT/A04/038 A/W O.L	2004	Jayendra kiran K. (Jkiran)

Result Sign Off

	Sign Off Date	Sign Off Reason
1	04-10-2025 16:10:07 IST	Sign Off Level 1, Reason: Data Submitted for review
2	04-10-2025 16:33:05 IST	Sign Off Level 2, Reason: Review

System Name NAL_ARD_HPLC_04_PDA

Reported by User: Manikanta.Bheemavarapu (Manikanta.B)

Report Method: General Report_DNT

Report Method ID: 1358

Page: 2 of 2

Project Name: 2025\October\NAL_ARD_HPLC_04

Date Printed:

04-10-2025

16:37:46 Asia/Kolkata