


SAMPLE INFORMATION

Sample Name:	DA003-PPA/A02/016 Dry solid	Acquired By:	Manikanta
Sample Type:	Unknown	Sample Set Name:	17102025_HPLC_03_S001
Vial:	1:B,5	Acq. Method Set:	17102025_HPLC_03_PPA_2_MTH
Injection #:	1	Processing Method:	17102025_HPLC_03_P006
Injection Volume:	10.00 ul	Channel Name:	W2489 ChA
Run Time:	36.0 Minutes	Proc. Chnl. Descr.:	W2489 ChA 213nm
Date Acquired:	17-10-2025 13:52:37 IST	Column_ID:	NAL-ARD-LC-2024-001
Date Processed:	17-10-2025 14:59:14 IST	AR.Number	HPLC/2510/695
Batch Number:	DA003-PPA/A02/016	Instrument ID:	NAL_ARD_HPLC_03

METHOD INFORMATION:

Column name:XBridge C18(50*4.6)mm,3.5um
 Mobile phase A:0.1% TFA IN1000ml H2O
 Mobile phase B: 0.05%TFA IN 1000ml ACN
 Gradient (%B) :0/30,5/30,25/90,35/90,36/30,42/30
 Column Temp :40°C
 Sample Temp :25°C
 Wavelength :220nm
 Run time :42 min

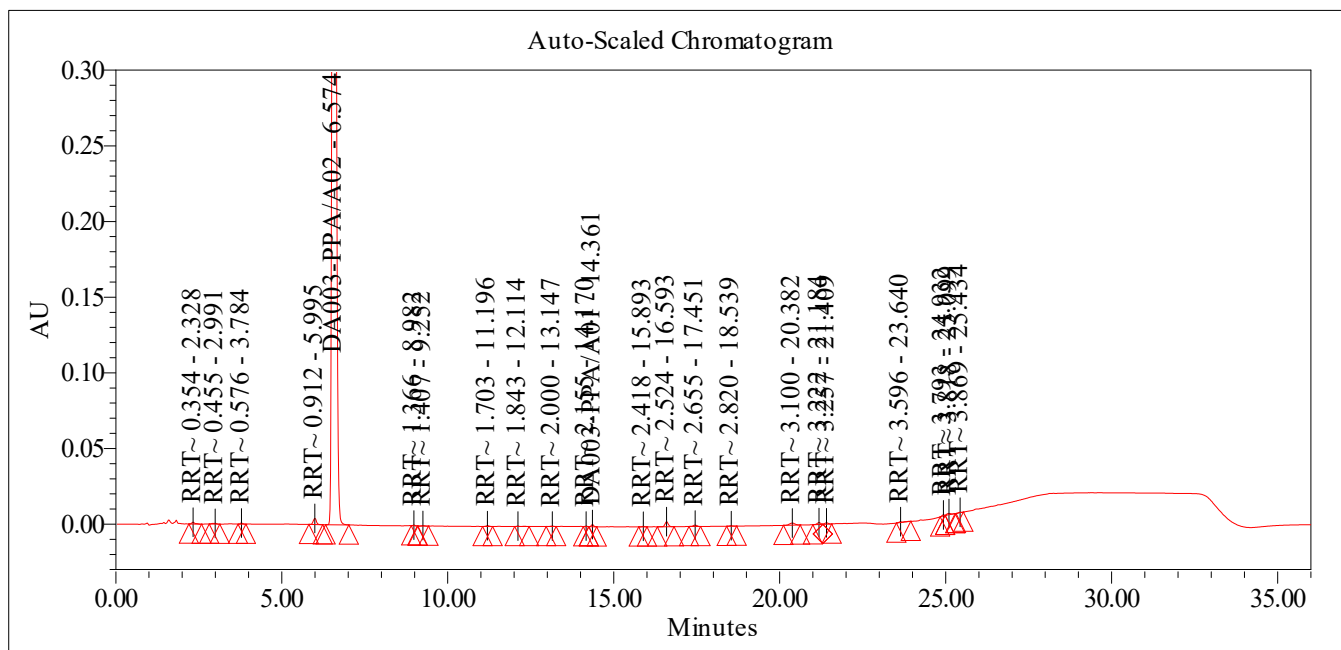

Peak Results

	Name	RT	Height (μV)	Area	% Area	RT Ratio
1	RRT~ 0.354	2.328	1236	8534	0.10	0.35

Peak Results

	Name	RT	Height (μ V)	Area	% Area	RT Ratio
2	RRT~ 0.455	2.991	517	5028	0.06	0.46
3	RRT~ 0.576	3.784	772	4154	0.05	0.58
4	RRT~ 0.912	5.995	4106	27176	0.33	0.91
5	DA003-PPA/A02	6.574	1193374	8019203	98.18	1.00
6	RRT~ 1.366	8.982	448	2171	0.03	1.37
7	RRT~ 1.407	9.252	307	2047	0.03	1.41
8	RRT~ 1.703	11.196	494	3147	0.04	1.70
9	RRT~ 1.843	12.114	242	2445	0.03	1.84
10	RRT~ 2.000	13.147	322	1881	0.02	2.00
11	RRT~ 2.155	14.170	373	1728	0.02	2.16
12	DA003-PPA/A01	14.361	1515	7874	0.10	2.18
13	RRT~ 2.418	15.893	329	1728	0.02	2.42
14	RRT~ 2.524	16.593	3367	22354	0.27	2.52
15	RRT~ 2.655	17.451	909	7291	0.09	2.65
16	RRT~ 2.820	18.539	266	1968	0.02	2.82
17	RRT~ 3.100	20.382	1470	16648	0.20	3.10
18	RRT~ 3.222	21.184	1222	9049	0.11	3.22
19	RRT~ 3.257	21.409	924	6661	0.08	3.26
20	RRT~ 3.596	23.640	586	6289	0.08	3.60
21	RRT~ 3.793	24.932	618	3002	0.04	3.79
22	RRT~ 3.818	25.099	748	6194	0.08	3.82
23	RRT~ 3.869	25.434	304	1488	0.02	3.87

Result Sign Off

	SampleName	Result Id	Sign Off Full Name	Sign Off Date
1	DA003-PPA/A02/016 Dry solid	3952	Raja Relangi (raja)	17-10-2025 14:59:42 IST

Result Sign Off

	Sign Off Reason
1	Sign Off Level 1, Reason: Data Submitted for review

System Name NAL_ARD_HPLC_03